

NEUROBLATE ROBOTIC PROBE DRIVER


LOW PROFILE DELIVERY PLATFORM
FOR ROBOTIC LASER THERMOTHERAPY

Precise robotic linear positioning prevents
laser probe misplacement

Probe can be directed from the work
station during the procedure

Hands-off laser manipulation eliminates
multiple trips into the MR scan room
and procedure delays



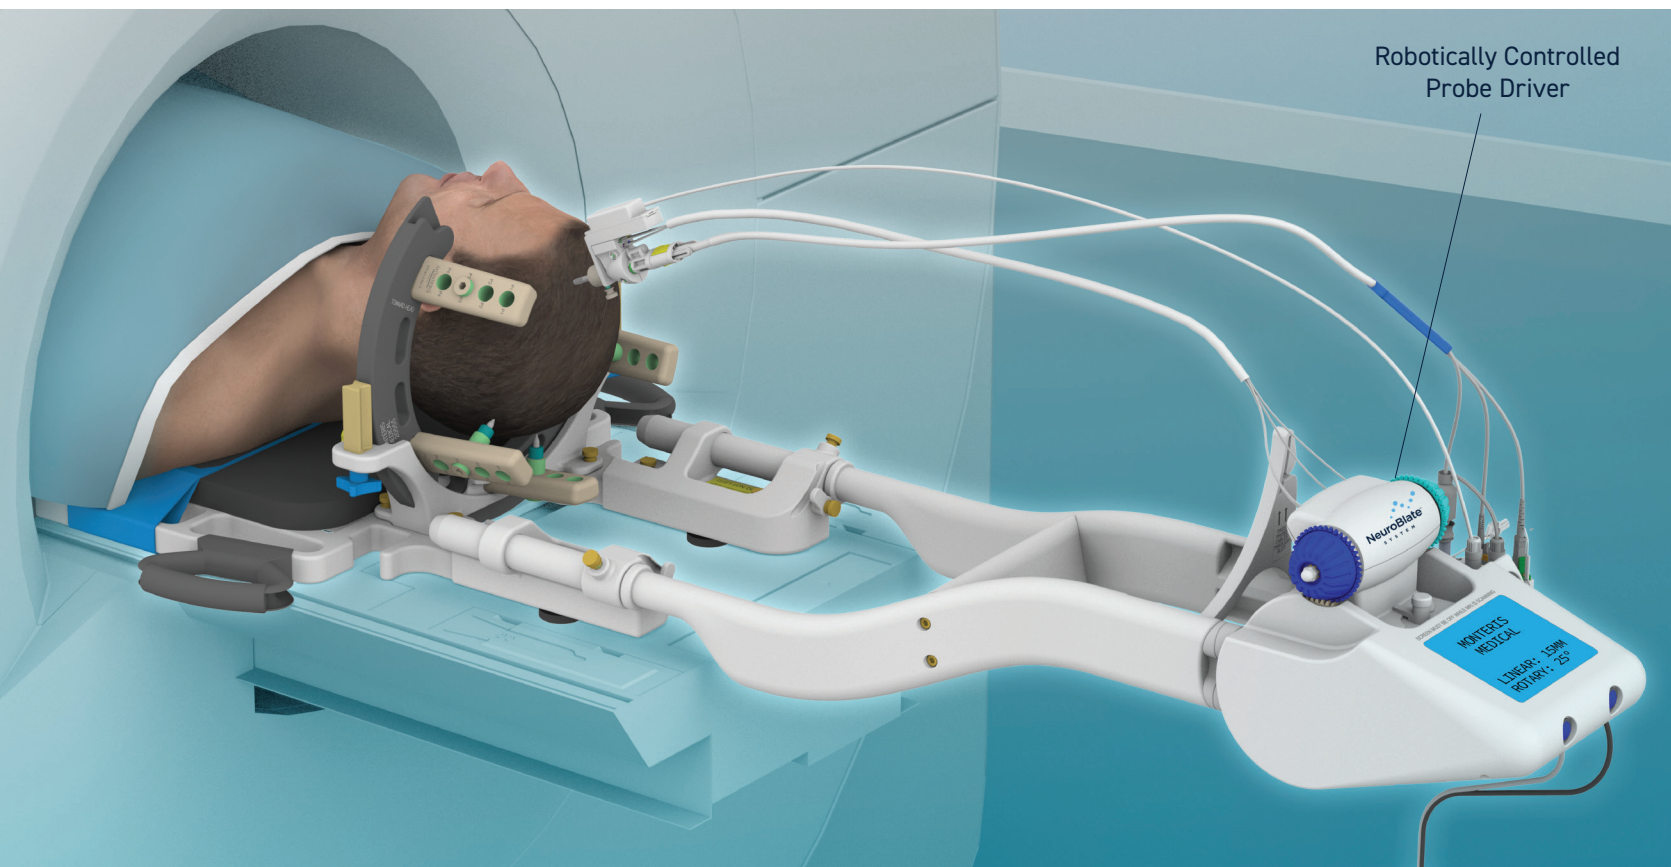

Robotically Controlled
Probe Driver

EXPANDED CRANIAL ACCESS

The Robotic Probe Driver, designed for use with a skull anchor like the Monteris Mini-Bolt, reduces profile in the MRI for access to virtually any brain location along the ideal trajectory.

PROBE DRIVER

RPD-01: NeuroBlade® Robotic Probe Driver

NBD-01: ADP(Advanced Probe Driver)*

DISCLOSURES:

The NeuroBlade® System is intended for ablating intracranial soft tissue, including brain structures. Patients must be able to undergo MRI exposure and be surgical candidates. The technology is not appropriate for every lesion type and location. It may be difficult to use the technology on certain large or irregularly shaped lesions.

All brain surgeries carry risk. Possible adverse events include, but are not limited to, hematoma, embolic events, edema, bleeding, unintended major tissue damage and permanent neurological deficits. Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions and potential adverse events. For full prescribing information, please visit monteris.com.

Contact Monteris Medical Corporation for more information.
Not available for sale outside the U.S. or Canada.

*For use with stereotactic Mini-Frame only

U.S. Office

14755 27th Ave. N., Suite C
Plymouth, MN 55447, USA
+1.866.799.7655

Canadian Office

Unit 1B-25 Scurfield Blvd.
Winnipeg, MB R3Y1G4, Canada
+1.204.272.2220

monteris.com

Rx Only

©2019 Monteris. All Rights Reserved. ™ and ® denote Trademarks and Registered Trademarks of Monteris Medical Corporation.

 **MONTERIS**
MEDICAL

AA10121 Rev C.2 10/19